

NATURAL ROCK SAMPLE

Performance Monitoring Accessory for the RAD7
User Manual

TABLE OF CONTENTS

TABLE OF CONTENTS	2
1 INTRODUCTION	3
2 RAD7 RADON SENSITIVITY CHECK	4
2.1 Purge the RAD7	5
2.2 Hook up to the Natural Rock Sample	5
2.3 Start a 3-Hour Test	5
2.3.1 Drying and Resealing the Natural Rock Sample	5
2.4 Radon Data Assessment	6
2.5 Multiple RAD7s	8
2.6 Cumulative Spectrum	9
3 RAD7 THORON SENSITIVITY CHECK	10
3.1 Thoron Measurement	10
3.1.1 Radon Interference	10
3.2 Rough Thoron Check	11
3.3 Better Thoron Check	11
3.3.1 Experimental Protocol	13
3.3.2 Calculation	13
3.3.3 Assessing The Thoron Data	13

1 INTRODUCTION

The Natural Rock Sample is a 21oz (600g) sample of granite gravel, enclosed in a container that may be sealed using a pair of ball valves and end caps.

Granite generally contains trace amounts of both uranium and thorium that has been in the rock since it was formed, millions if not billions of years ago. Therefore all the progeny of both the uranium and thorium decay chains are fully supported and in full equilibrium down to ^{226}Ra and ^{224}Ra .

When the Natural Rock Sample is kept dry, it constitutes a rock-steady emitter of both radon and thoron. This manual shows how to take advantage of that property to check the performance of a RAD7. Please note that to keep the emission constant it is essential that the Natural Rock Sample be kept fully dry. This is because the radon and thoron emanation efficiency depends upon the humidity at the rock-air interface on the surface of the rocks. Always use a Small Drying Tube, with blue, active desiccant in it, in the closed-loop radon calibration circuit, or upstream of the desiccant in the open-loop thoron calibration configuration. If the desiccant in the Small Drying Tube gets used up it should be replaced or regenerated. The Natural Rock Sample should be thoroughly dried by purging with dry air every 30 - 50 days. This can be done as part of the standard radon calibration check protocol (see Section 2.3.1) or, if no calibration check is required, as a standalone procedure. The Natural Rock Sample has a desiccant pack and humidity indicator built into it for maintaining and verifying dryness. For thoron sensitivity measurement, the carrier air, pushing the thoron into the sample path, should be dried before it enters the rock sample. These configurations are illustrated on the following pages.

After calibration at DURRIDGE Company, and with the optional Thoron Calibration Check Kit, the Natural Rock Sample can be used for low-precision checking of both the radon and thoron sensitivities of any RAD7. The Natural Rock Sample can provide a means for monitoring long-term changes in both radon and thoron sensitivity.

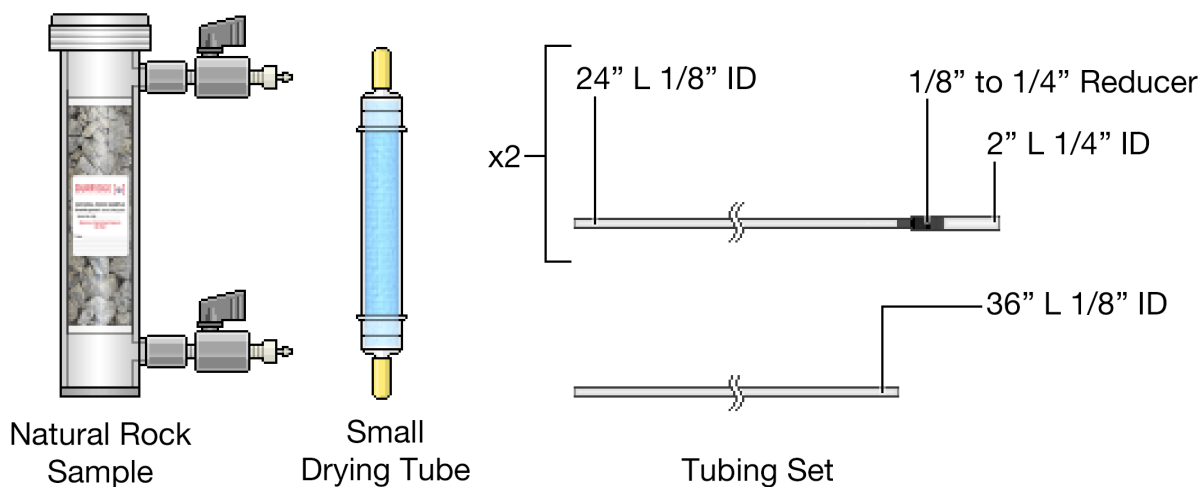


Figure 1 Natural Rock Sample Components

2 RAD7 RADON SENSITIVITY CHECK

After sitting sealed on a shelf for one month, the radon in the Natural Rock Sample container will have reached within 1% of a steady value, in which the rate of emission of radon into the container is equal to the rate of loss by decay and leakage. If that quantity of radon is known, and if it is distributed around an air loop of known volume, then the radon concentration in the air is known. If one of the devices in the air loop is a RAD7, the RAD7's reported radon concentration may be compared with the known concentration, and thus the sensitivity of the RAD7 may be effectively checked. A correction may be applied to the Natural Rock Sample radon reading to account for the ambient air radon concentration (see Section 2.4).

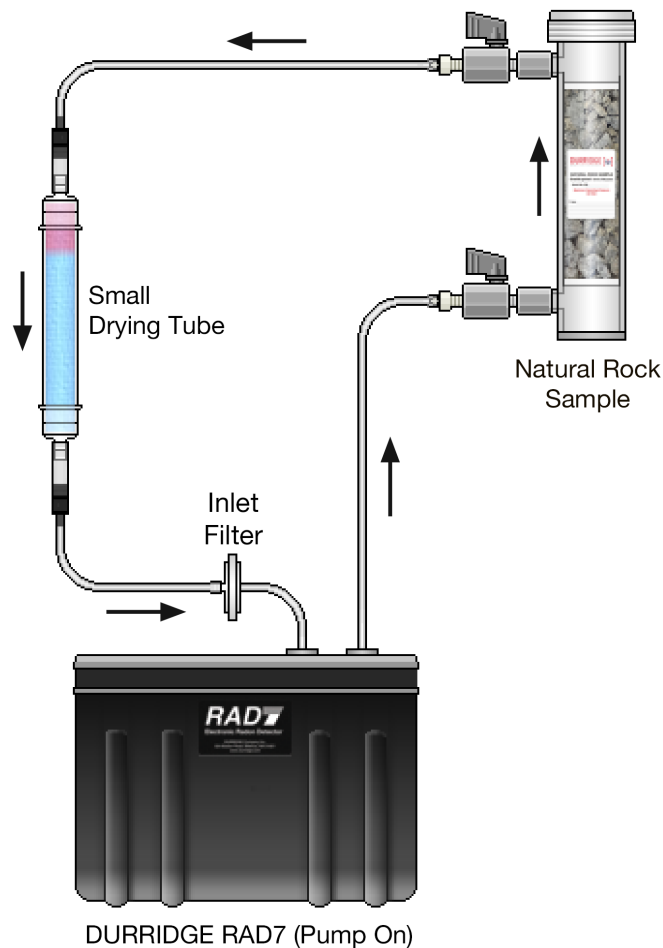


Figure 2 Radon Sensitivity Check Setup

In practice, provided the device and tubing configuration is identical to the calibration setup, all that is required to check the RAD7 sensitivity is to compare the 'standardized' average RAD7 reading (see below) with the standardized average reading on the Natural Rock Sample calibration certificate. The ratio of the two will give a correction factor that may be applied directly to RAD7 readings.

2.1 Purge the RAD7

First, purge the RAD7 with dry air in an open loop for at least 5 minutes, then switch to 1-day protocol: select Setup, Protocol, 1-day, and push [ENTER]. Start a reading, still sampling fresh air through a drying unit. Go to the third status window (push the [Menu] key, then push [ENTER], [ENTER], Rt Arrow, Rt Arrow, and observe the relative humidity in the top right corner. Keep the reading going until the RH is below 9%, then switch off the RAD7.

If a correction is to be made to the Natural Rock Sample radon reading for radon added to the air loop by the ambient air, after purging the RAD7, (see section 2.4), the fresh-air measurement should be kept going until at least one and preferably two or three cycles are completed.

2.2 Hook up to the Natural Rock Sample

Hook the RAD7 up to the Natural Rock Sample in a closed loop, using the tubing and Small Drying Tube provided with the Natural Rock Sample. Use the configuration shown in Figure 2, with the Small Drying Tube upstream of the RAD7, and the Natural Rock Sample connection upstream of the Small Drying Tube. If one end of the Small Drying Tube has started to turn pink, indicating that it is wet, that end should be positioned closest to the RAD7 outlet.

2.3 Start a 3-Hour Test

Switch on the RAD7 and press the menu key. Select 1-day protocol (Setup, Protocol, 1-day, [ENTER]). Change the Recycle number to 6 (Setup, Protocol, Recycle, 06, [ENTER]). Put the RAD7's infrared printer in place and switch off the RAD7.

Switch on the RAD7 printer. Switch on the RAD7 and let it print out the header, including a review of the settings. Check the printed review to make sure the Cycle time is 00:30 (30 minutes) and the Recycle number is 06. Open the ball valves on the Natural Rock Sample container and start a test (Test, Start, [ENTER]).

Keep the measurement going until all six cycles are complete and the summary is printed out (3 hours). Average the last four readings. Record that average with the date. If a thoron test is to be conducted (see Section 3), the best time to do it would be 1 - 2 hours after the radon check (see Section 3.1.1 for details).

2.3.1 Drying and Resealing the Natural Rock Sample

After testing is complete, the Natural Rock Sample should be thoroughly dried and prepared for storage. To do this, set up the Natural Rock Sample in a closed loop with a RAD7 and a laboratory drying unit containing fresh desiccant. (At this point the Small Drying Tube that was used in the 3-hour test should be sealed with yellow caps and set aside until the next 3-hour test is conducted.) The Natural Rock Sample should be positioned downstream of the laboratory drying unit, and the laboratory drying unit should be connected with the end furthest from the screw cap connected to the Natural Rock Sample. The screw cap end, which may be pink (indicating that it is wet), should be connected to the RAD7 outlet as shown in Figure 3, on the following page.

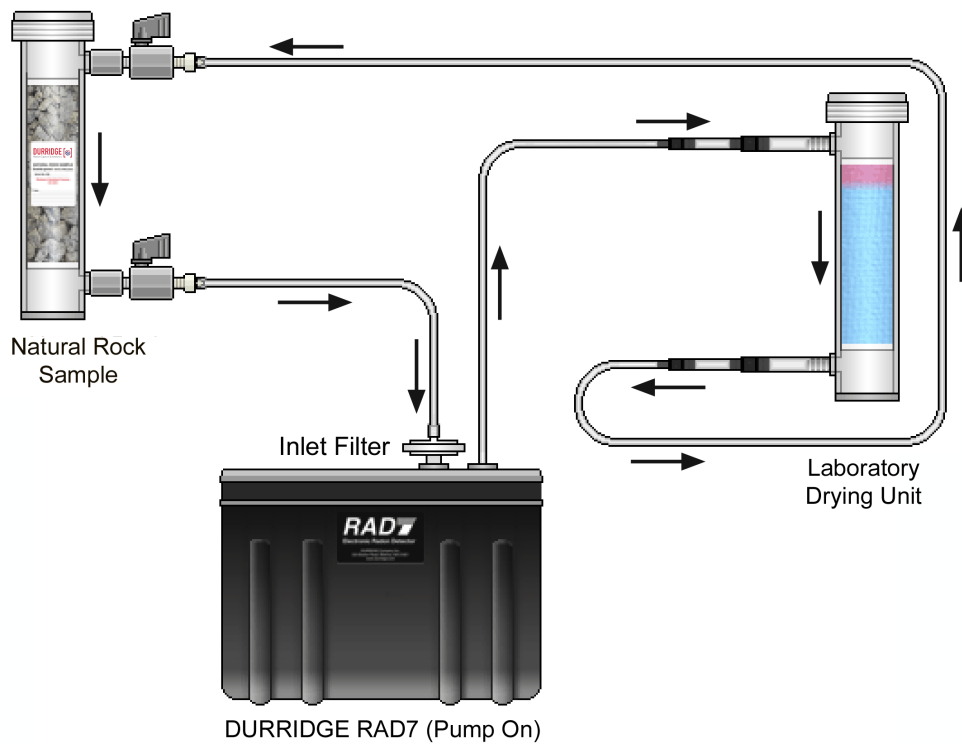


Figure 3 Natural Rock Sample drying loop configuration

Set the RAD7 pump to 'ON' (Setup, Pump, On [ENTER]), go to third status window (Setup, Enter, Enter, Rt. Arrow, Rt. Arrow.) and monitor the RH reading. Keep the air circulating through the loop until the relative humidity (RH) drops to 4% or below. The drying process may take many hours.

Once the RH stays at 4% or below, turn off the pump (Setup, Pump, Off [ENTER]), close the ball valves, disconnect the tubing, and insert the end caps on the Natural Rock Sample tube. Mark the date on the label and store the Natural Rock Sample with its tubing and Small Drying Tube on a shelf for between 30 and 50 days before repeating the process.

If the ball valves are opened for any reason on a later date, remove the old label and replace it with a new label showing the last date on which the valves were closed, and left closed. The rock sample will be ready for another radon check not before one month from that date. The next measurement should be made within 50 days of the date on the label, to avoid the risk of moisture creeping in and changing the emanation efficiency, and hence the radon and thoron output, of the Natural Rock Sample.

2.4 Radon Data Assessment

If the Natural Rock Sample was never calibrated, keep the average of the last four readings (3, 4, 5, and 6) in a record for future reference. (Figure 4 on the next page shows a typical data set in DURRIDGE's CAPTURE software, with the last four readings selected.) Every standard RAD7 should produce nearly the same result with that Natural Rock Sample if its sensitivity is as calibrated and if the rock sample is dry and has been sealed for between 30 and 50 days. For greater reproducibility, 2/3 of the ambient air radon concentration can be subtracted from the averaged readings to correct for the residual radon in the air in the system after purging. However, if the ambient radon concentration in the air is less than 100 Bq/m³ (2.7 pCi/L) the error introduced by ignoring it will be less than 1%.

If the Natural Rock Sample has been calibrated by DURRIDGE Company, the calibration certificate gives the standardized average of readings 3, 4, 5 and 6, obtained with the standard setup, a well purged and dry RAD7 and 30-minute cycles. Thus the ratio of the value stated on the rock sample calibration certificate to the measured standardized average gives you the correction factor directly. RAD7 readings multiplied by that ratio will give readings consistent with the DURRIDGE calibration system to within 15%.

You may also, if you wish, calculate the total radon amount in the air loop, and hence originally in the Natural Rock Sample container. If the radon amount is R_n and the volume of the air loop is V , then the radon concentration is R_n/V . The air volume in the Natural Rock Sample is about 460ml, a standard RAD7 is 800ml, and the tubing with small drying tube is 16ml, for a total volume of a standard Natural Rock Sample system with standard RAD7 of 1.275 L. If R_n is expressed in pCi, then the radon concentration will be $R_n/1.275$ pCi/L. If R_n is expressed in Bq, then the radon concentration will be $R_n/1.275$ Bq/L, or $1000 * R_n / 1.275$ Bq/m³.

In pCi, $R_n = 1.275 * \text{radon concentration in pCi/L}$.

In Bq, $R_n = 0.001275 * \text{radon concentration in Bq/m}^3$

If the certified and observed standardized average values differ by more than 15%, we recommend that the RAD7 be returned to DURRIDGE Company for service. If, after several monthly sensitivity checks, there is a consistent ratio between the observed and the certified standardized average radon concentration, you may consider applying a multiplier to all readings made with that RAD7, to bring them in line with the Natural Rock Sample standard. If you notice a big jump, up or down, in the reading, from the previous month, first look to see if the RAD7 was properly purged before the measurement was started. If there is no obvious reason for the jump, the RAD7 should be returned to DURRIDGE for service.

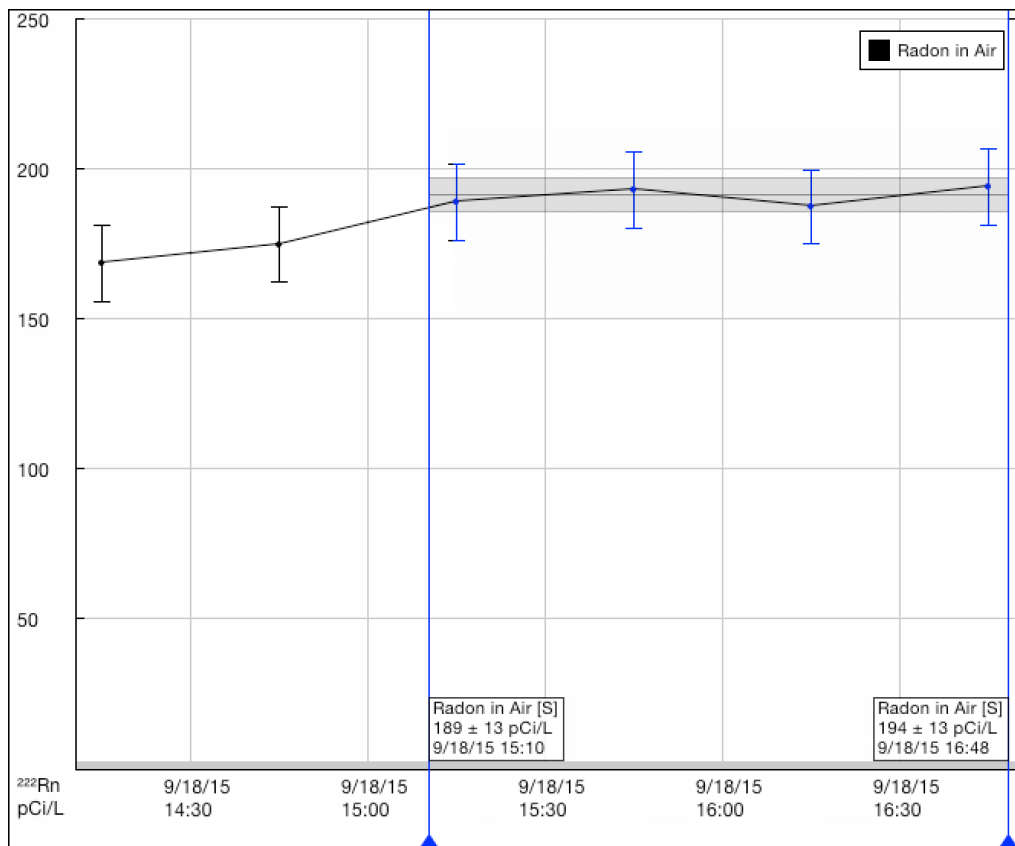


Figure 4 Graph of Natural Rock Sample sensitivity test data

2.5 Multiple RAD7s

Before using the Natural Rock Sample to check a RAD7's radon sensitivity, the Natural Rock Sample must be left sealed for a month, in order for the radon inside the container to reach equilibrium. That means a RAD7 can have its sensitivity checked each month on a regular basis. However, there is nothing to stop us hooking up multiple RAD7s in series in the loop connected to the Natural Rock Sample. This increases the volume of the loop and hence decreases the radon concentration in the loop, but by a predictable and reproducible amount. This method is recommended for checking up to six RAD7s on a monthly basis.

For the sake of argument, using rounded figures, let us assume that the total activity of radon inside the Natural Rock Sample container, when in equilibrium, is equal to 2 Bq. Let us also assume that the Natural Rock Sample and tubing has an air volume of 500ml while a RAD7 is 1L. Then when the RAD7 is connected up to the Natural Rock Sample and the radon distributed around the loop, the radon concentration will be $2 / 1.5 = 1.333 \text{ Bq/L} = 1333 \text{ Bq/m}^3$. If every additional RAD7 adds 1L to the loop, then four RAD7s would total 4.5L, including the Natural Rock Sample and tubing. The radon concentration in the loop would then become $2 / 4.5 = 0.444 \text{ Bq/L} = 444 \text{ Bq/m}^3$. While this is less than 1333 Bq/m^3 , it is still enough to make a good reading in two hours and a high precision reading in 12 hours.

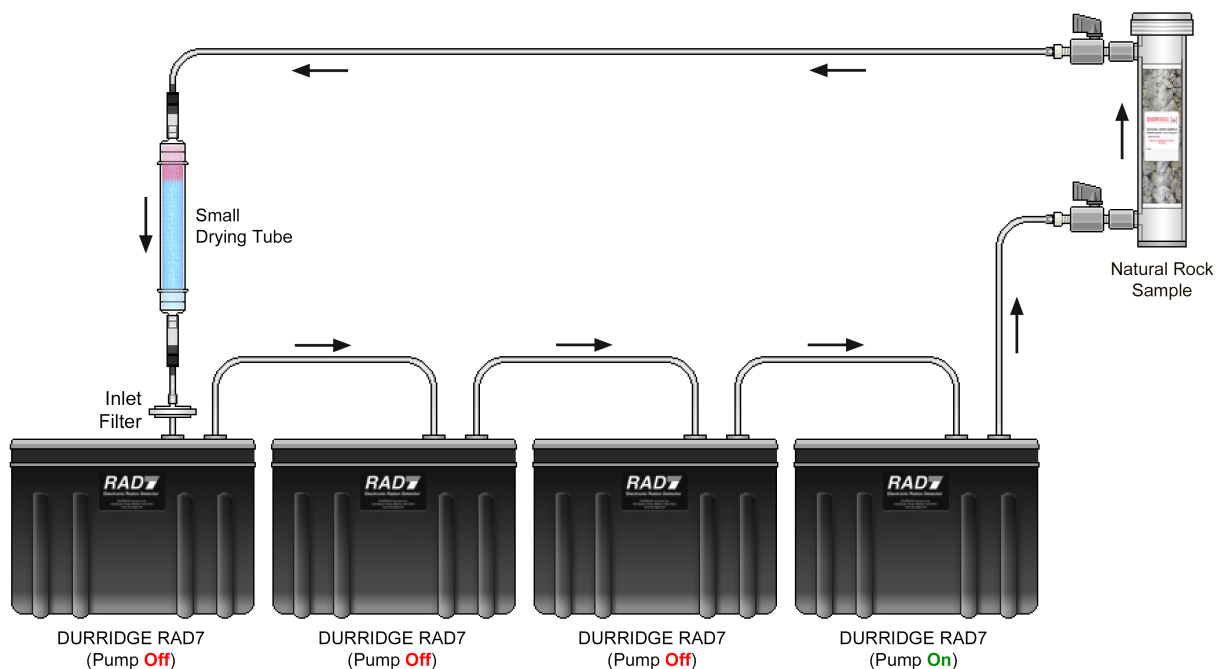


Figure 5 Multiple RAD7 Sensitivity Check Configuration

Each month, all four RAD7s can be connected in series with one another and thoroughly purged and dried out, before being connected to the rock sample to obtain a sensitivity check. Each month the setup should be identical, with the same number of RAD7s and the same pieces of tubing to connect up the entire loop. During the measurement all the RAD7 pumps, except one, should be set to OFF (Setup, Pump, Off, [ENTER].)

If any of the RAD7s had developed a leak, the radon concentration in the loop would fall rapidly. Thus in addition to keeping a record of the average readings during the check, for each month, a record of

the slope of the average for all RAD7s should also be maintained, as the radon concentration falls off over time from decay and any leakage. If during one month the slope is steeper than usual, that would be an indication of a leak in the loop somewhere.

Although it is possible to combine several RAD7s in a loop for monthly radon sensitivity checks, this technique will not work for checking thoron sensitivity, due to the decay of thoron in the air as it travels around the loop (see Section 3.1). However, there is no need to wait between successive thoron checks, and all the RAD7s can undergo the rough thoron check individually, sequentially, without any delay between measuring the thoron response of one RAD7 and the next. The monthly protocol may therefore be:

1. Connect all RAD7s in series, set all protocols to 1-day, set all pumps, except one, to OFF. Put a Laboratory Drying Unit upstream of the line, with one end open to fresh air.
2. Set the RAD7 with an active pump to Purge, for 15 minutes, to purge all residual radon out of the RAD7s and start to dry them out.
3. Select **Test, Start**, [ENTER] on all RAD7s, starting a 1-day test in each of them (with only one pump operating).
4. After at least two cycles (1 hour), or preferably 3 cycles (1.5 hours), stop the tests.
5. Disconnect the Laboratory Drying Unit. Connect the string of RAD7s to the Natural Rock Sample and Small Drying Tube.
6. Open the valves and select **Test, Start**, [ENTER] on all RAD7s (all still in 1-day protocol and with all pumps, except one, set to OFF).
7. Depending on the precision required, after between 3 and 24 hours, the tests may be stopped and the RAD7s disconnected.
8. If required, rough thoron checks may then be performed with each RAD7, separately connected to the Natural Rock Sample. Wait 1-2 hours before doing this, to allow time for the C window radon counts to decay away (see Section 3.1.1).
9. Careful notes should be kept of all actions and readings, and all data downloaded from each RAD7 to a computer using DURRIDGE's CAPTURE software.
10. The Natural Rock Sample should be thoroughly dried and stored for 30 - 50 days, using the procedure described in Section 2.3.1, before making the next calibration check.

2.6 Cumulative Spectrum

It is important that the cumulative spectrum (based on counts from multiple cycles) be printed and inspected periodically. It gives excellent diagnostic information on the health of the instrument. Using the Natural Rock Sample to check the calibration of the RAD7 every month is a convenient opportunity to inspect the cumulative spectrum. With the Recycle set to 6 cycles, as indicated above, at the end of the sixth cycle the RAD7 will automatically finish the run and print out a run summary. This consists of some data, a bar chart of the six readings and then the cumulative spectrum. That spectrum should show a sharp peak in the A window, about midway between the boundaries. There may also be peaks in the other three windows and at 5.3 MeV (210-Po) just to the left of the A window. Please see the RAD7 manual for a description and image of some possible pathological spectra to watch out for.

3 RAD7 THORON SENSITIVITY CHECK

3.1 Thoron Measurement

The RAD7 is capable of making a direct measurement of thoron gas concentration in air. It does this by counting ^{216}Po decays inside its measurement chamber. However, Thoron has a short half life, 55.6s, so most of the thoron in the sample will be lost during acquisition if the time from sampling to entering the measurement chamber exceeds even a minute. Therefore when measuring thoron the sample acquisition time must be as short as conveniently possible, and always consistent. Additionally, the exact same setup should be used for thoron calibration as for thoron measurement. This setup necessarily involves a specific length of tubing and a Small Drying Tube full of desiccant, as the RAD7 is less sensitive in a humid environment. Just as with radon, the Natural Rock Sample's thoron output is a function of humidity at the rock-air interface, so it is important to ensure that your Natural Rock Sample is thoroughly dried out before making a measurement.

The setup assumed in the RAD7 data processing and stated as standard in the manual consists of a Small Drying Tube, which may be used as a wand for sniffing, along with a standard input tubing of 36" (91.4cm) length and inner diameter of 3/16" (4.8mm), as shown below.

This typically gives the RAD7 a thoron sensitivity of about half its radon Sniff sensitivity. The ^{216}Po daughter of thoron has only a 145mS half life so the main component in the response time of the RAD7 to a step change in thoron concentration is the time taken to acquire the sample. The response is virtually instantaneous.

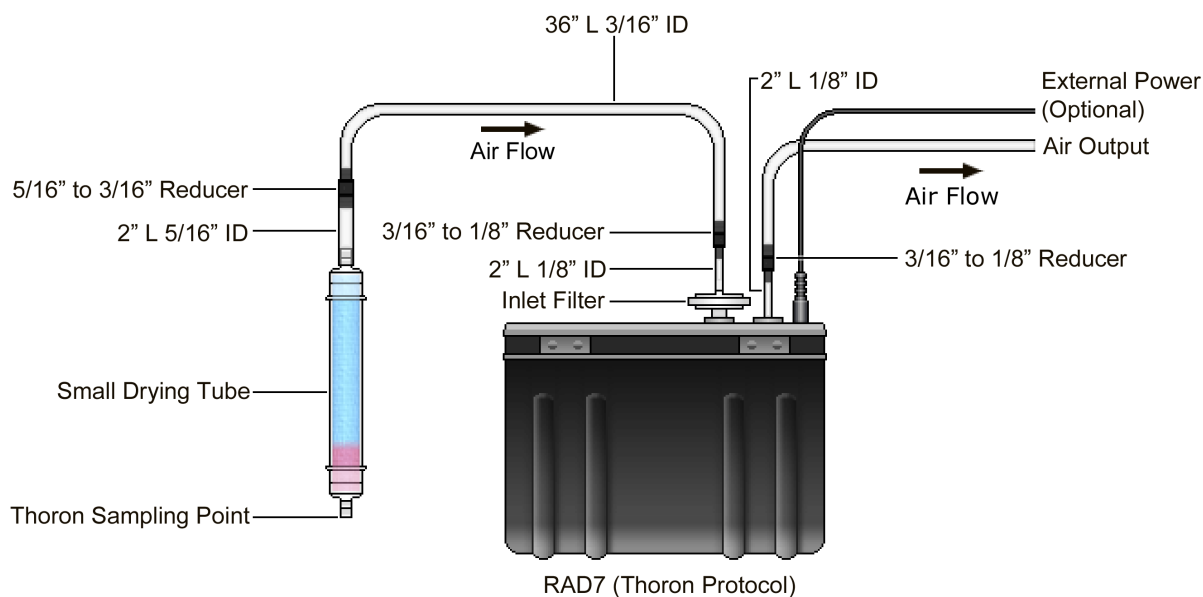


Figure 6 Thoron Measurement Standard Setup

3.1.1 Radon Interference

The alpha particle from ^{216}Po decay has an energy of 6.78 MeV, which is between the ^{218}Po and ^{214}Po peaks in the ^{222}Rn decay chain. That places it within the B window of the RAD7 spectrum, while the ^{214}Po peak lies in the C window. About 1% of the ^{214}Po counts are in a low energy tail from the peak, and spill into window B. The spill factor is measured during calibration and the count in window B is corrected for that spill by the RAD7 and by DURRIDGE's CAPTURE software when calculating the

thoron concentration. Nevertheless, the presence of a large spill from window C would increase the uncertainty of the thoron count in window B. It is therefore important that the C window count be low when performing a thoron measurement or calibration.

If a radon calibration check of a RAD7 has been performed with a Rock Sample, it is good practice to wait an hour or two for the count rate in window C to drop below 10 cpm, before proceeding with the thoron calibration check. During this time, the Natural Rock Sample can be left purging with a RAD7 (set Test > Purge) and a Laboratory Drying Unit, which will ensure that the Natural Rock Sample is thoroughly dry before the measurement begins.

3.2 Rough Thoron Check

Before closing the ball valves and disassembling the setup, change the protocol to Thoron by selecting Setup, Protocol, Thoron, [ENTER]. Then turn the RAD7 off and back on, and let the printer print out the new header for thoron.

Start a measurement. Let it run for at least 15 minutes (3 five-minute cycles), or more if you would like a higher precision average. Average all the thoron readings. Store the thoron average reading with the radon average.

This thoron reading cannot be used to check the thoron sensitivity of the RAD7, as the reading is heavily dependent on the pump flow rate and even the position of items in the setup. For example, if the desiccant is placed upstream instead of downstream of the Natural Rock Sample it will make no difference to the average radon reading, but will make a big difference to the thoron readings. Even just switching the connections to the Natural Rock Sample can affect the thoron readings. However, if the setup remains identical in every respect from one monthly check to the next, if the RAD7 pump is still working at close to the same flow rate, and if the inlet filter is not blocked, then thoron readings made with this setup will be similar from one month to the next. After several months of experience the user will know the typical variation and will recognize an anomalous shift, should it occur.

3.3 Better Thoron Check

A more accurate thoron sensitivity check involves the Thoron Calibration Check Kit, which is sold separately. To check the thoron sensitivity of a RAD7 using this kit, the measurement must be made in precisely the same conditions and using the same configuration as thoron measurements in regular use. In standard thoron protocol, the RAD7 has 1m of 3/16" ID tubing between the inlet filter and a Small Drying Tube, which may be used as a wand for sniffing purposes.

The thoron check process therefore requires that the sampling point at the end of the Small Drying Tube must be open to the air. It is the thoron concentration at that sampling point that we measure. Thus we put a T-connector at that location, inject thoron at a known rate, using a carrier with less than the RAD7 flow rate, and with fresh air from the other side of the T-connector supplying the balance of air to make up the RAD7 flow rate. This configuration is illustrated in Figure 7.

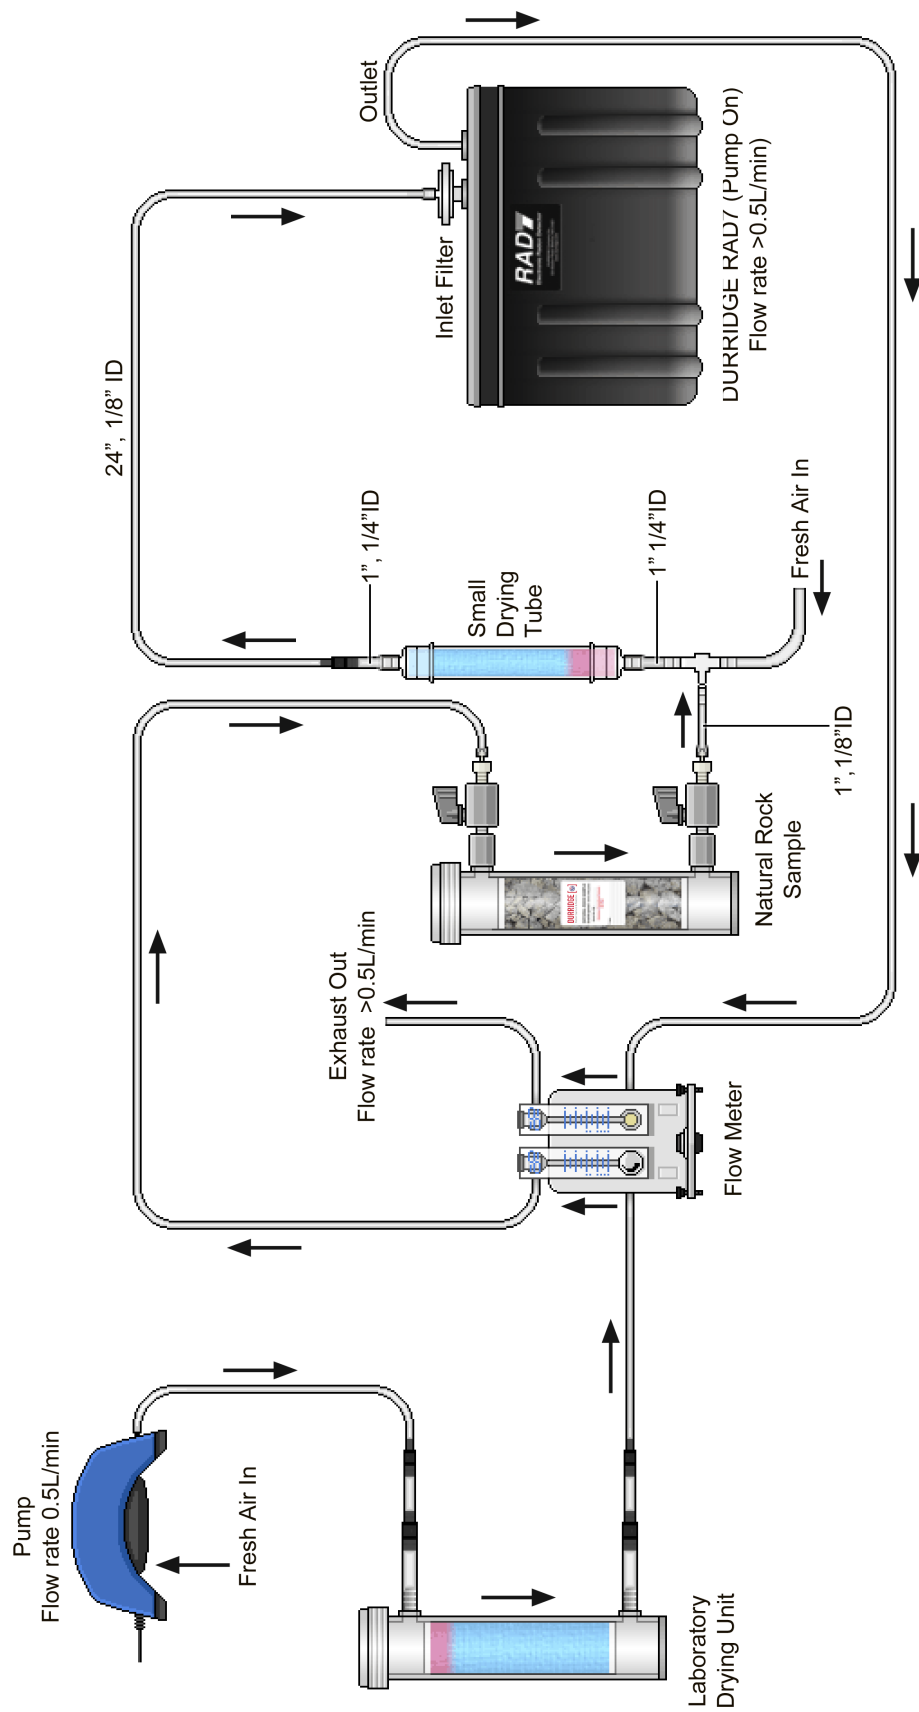


Figure 7 Thoron Sensitivity Check configuration

3.3.1 Experimental Protocol

- a) Set up the experiment exactly as in the diagram above, or else with the RAD7 sampling path in exactly the same setup as will be used for measuring thoron.
- b) Adjust the flow rate through the Natural Rock Sample to 0.55 L/min. A flow rate of 0.55 L/min is chosen as a standard flow rate for injecting thoron into the RAD7 sample path because that may be relied upon to be less than the RAD7 pump flow rate, which may range from 0.6 L/min to 1 L/min or higher. With the set up as shown in the diagram above, run the external pump and adjust the needle valve so that the air flowing through the Natural Rock Sample is 0.55 L/min.
- c) Move the flow meter to the RAD7 outlet. Remove the flow meter from its position between the needle valve and the Natural Rock Sample and reconnect the tubing so that the needle valve is connected directly to the Natural Rock Sample. Connect RAD7 outlet to the input of the flow meter. The external pump can be kept running during this maneuver.
- d) Change the RAD7 to thoron protocol. Use the default thoron protocol (Setup, Protocol, Thoron, [ENTER]), or choose the default and then change individual parameters (e.g. cycle time) as desired. Turn off the RAD7, turn on the printer, turn on the RAD7 and let it print out a header. Examine the header to make sure everything is OK.
- e) Start a reading: Test, Start, [ENTER].

3.3.2 Calculation

With an identical air flow rate (0.55 L/min) through the Natural Rock Sample and identical tubing attached to the T connector, for every thoron calibration check, the rate of injection of thoron into the sample flow will always be the same. Let this be Th . The units of Th are pCi per minute or Bq per minute.

If the RAD7 flow rate, measured at the RAD7 outlet, is V L/min, then the thoron concentration in the sample air flow at the sampling point (which is very close to the T connection) will be Th/V . If Th is expressed in pCi/min and V is in L/min then Th/V will be pCi/L. If Th is expressed in Bq/min and the flow is in L/min then Th/V will be Bq/L. To convert to Bq/m³ multiply by 1000.

3.3.3 Assessing The Thoron Data

For an uncalibrated Natural Rock Sample, note the average thoron reading and the RAD7 flow rate. Multiply the thoron reading by the flow rate to get Th , the rate of injection of thoron into the sample flow (for units of Bq/m³ and L/min, divide the product by 1,000 to get Bq/min). The experiment may be repeated as often as desired; there is no need to wait for any ingrowth. However, after conducting this experiment, the Natural Rock Sample must be left sealed for a month before a radon check may be performed. The obvious time to do this experiment is 1 - 2 hours after a radon check.

As an option, DURRIDGE Company will calibrate a Natural Rock Sample for thoron. With a setup as above and a flow rate of 0.55 L/min through the Natural Rock Sample, we give you the rate of injection of thoron into the RAD7 sample path. You may then divide that by the flow rate of the target RAD7 to obtain the thoron concentration at the sampling point. This may be compared with the thoron reading in the RAD7 and a correction factor derived.

Records of the radon and thoron readings should be kept safely for later reference and comparison.

DURRIDGE Company Inc.
900 Technology Park Drive
Billerica, MA 01821

Telephone: (+1) 978-667-9556
Fax: (+1) 978-667-9557
Web: www.durridge.com
Email: service@durridge.com

© Copyright 2020 DURRIDGE Company Inc. All rights reserved.

DURRIDGE, the DURRIDGE logo, and the Works with the DURRIDGE logo are trademarks of DURRIDGE Company Inc., registered in the U.S.

Revision 2021-02-15